

A novel means for detection of muscular activity.

Michael Winger BS¹, Don Yungher BS¹, JB Barr PT DPT², A Joseph Threlkeld PT PhD², William Craelius PhD¹

¹Department of Biomedical Engineering, Rutgers, The State University of New Jersey

²Department of Physical Therapy, Creighton University

Abstract

Motivation: Gait analysis with EMG is a difficult and often laborious process. An ideal interface should extract maximal information from the neuromuscular system (NMS) non-invasively and at the same time provide high-bandwidth bi-directional communication with the NMS. **Goal:** Develop a minimally-invasive technology which will monitor an individual's muscular activity through a simple and comfortable interface.

Design: The Myokinetic Interface (MKI) is a wearable sleeve array of force-sensitive resistors (FSR's) which decode in near real-time with linear trainable filters, to be worn comfortably around the distal limb, covering major muscle groups, recording their pressure distributions. **Results:** Close correlation between MKI and EMG was found in preliminary work on the application of MKI to the lower limb in gait analysis: MKI was found to be highly repeatable, less subject to high-frequency artifact, and offers a counterargument to the concept of electromechanical delay in skeletal muscle. **Projection:** We are currently adapting the technology to people with a spinal cord injury, Parkinson's Disease or following a stroke. The relative simplicity of the MKI makes it feasible for home use, general rehabilitation, and as a biofeedback aid for people with a variety of disabilities.

Introduction

The Myokinetic Interface (MKI) is a sleeve array of force sensitive resistors (FSR's), which slide easily over the major muscles of the limb to provide a high-fidelity pressure mapping of the muscles. By measuring the kinetic activity of the muscles through a wearable array of pressure sensors, the MKI system provides a means for quantifying the properties of muscle activation which is easy to don/doff, and does not require expertise to operate or interpret, using changes in muscle shape..

Methods

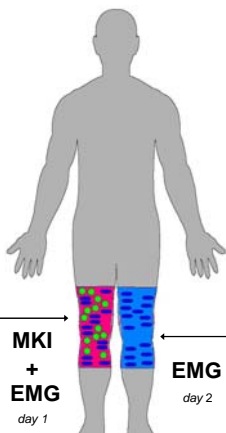


Figure: Subject donned MKI and EMG on same (day 1) and different (day 2) legs, and walked on a treadmill at 1.8, 3.0, and 6.0mph.

EMG **MKI**

Filter: ~3Hz

threshold

On/off times

ANOVA VR

-8 EMG tracks over the major anterior and posterior thigh muscles.

-33 MKI tracks: 17 ant/post thigh, 16 shank


-Healthy female, mid-20's, trained treadmill walker

-EMG and MKI on same (day 1) and different leg (day 2)

-EMG filtered with a simple 7-wt linear filter, MKI unfiltered.

Results

Muscle Activity Timing

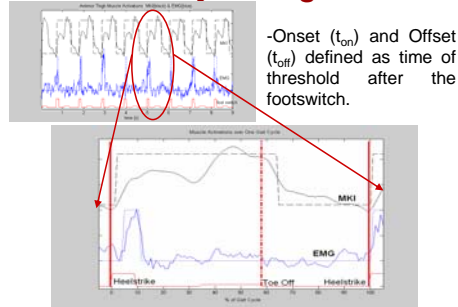

	EMG	MKI
t_{on} (msec)	18.8 ± 37.6	15.0 ± 5.35
t_{on} (% of cycle)	1.77 ± 3.54	1.41 ± 0.50

Timing of Muscle Activity Onsets, as measured by EMG and MKI, mean ± std.dev.

$$Z_{obs} = \frac{(\bar{X}_1 - \bar{X}_2) - (\mu_1 - \mu_2)}{\sigma_{\bar{X}_1 - \bar{X}_2}} \quad Z_{obs} = 0.2648 \ll \pm 1.96 \quad \alpha=0.05$$

Repeatability

The Variance Ratio (VR) quantifies the repeatability¹ of the wave-forms over multiple (8) gait cycles:

$$VR = \frac{\sum_{i=1}^k \sum_{j=1}^n (X_{ij} - \bar{X}_i)^2 / (k(n-1))}{\sum_{i=1}^k \sum_{j=1}^n (X_{ij} - \bar{X})^2 / (kn-1)}$$

	VR	Variance Ratio (where identical signals → 0 and random noise → 1) calculated for EMG and MKI.
MKI	0.028	
EMG(raw)	0.877	
EMG(enveloped)	0.555	

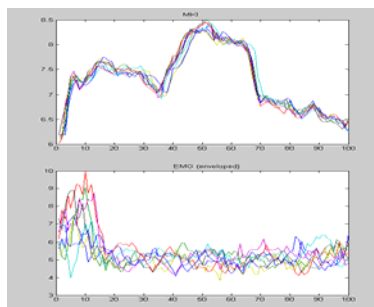


Figure: Overlays of signals from eight gait cycles: raw MKI (top) and EMG (bottom)
-MKI is demonstrably more repeatable than EMG.

¹Hwang, Ing-Shiou, et al. "Electromyographic Analysis of Locomotion for and Hemiparetic Subjects". *Gait and Posture* 18. (2003): 1-12

Compatibility

-Timing statistics for the 3mph:

	EMG (msec)(mean ± s.d.)	MKI (msec)(mean ± s.d.)
t_{on}	18.8 ± 37.6	15.0 ± 5.35
t_{off}	129 ± 24.2	691 ± 8.35
duration	110 ± 38.9	676 ± 7.44

	EMG (% of cycle)(mean ± s.d.)	MKI (% of cycle)(mean ± s.d.)
t_{on}	1.77 ± 3.54	1.41 ± 0.50
t_{off}	12.1 ± 2.28	65.1 ± 0.79
duration	10.4 ± 3.67	63.7 ± 0.70

-One-way classification (ANOVA) calculates the inter-rater compatibility between the MKI and EMG.

$$\bar{X} = \frac{1}{2n} \sum_i (\bar{X}_i) + \sum_i (\bar{Y}_i)$$

$$r^2 = \frac{\sum_i |(X - \bar{X})| \sum_i |(Y - \bar{Y})|}{\left(\sum_i |(X - \bar{X})|^2 + \sum_i |(Y - \bar{Y})|^2 \right)}$$

Results were calculated for two days at moderate speed, and one day at high speed over 9 steps:

	6mph	3mph(1)	3mph(2)
t_{on}	0.8764	0.8347	0.9586
t_{off}	0.9930	0.9905	0.9935
dur	0.9304	0.9896	0.9907

This correlation value indicates that there is reasonable-to-excellent agreement between methods for quantifying timing within the gait cycle, when systematic biases are eliminated.

Conclusion

- MKI is more repeatable than the standard means of detection of neuromuscular volition.
- MKI waveform outlasts EMG in-whole or in-part due to the muscle activation
- For timing, the EMG and MKI exhibit moderate to excellent compatibility.
- Z-score shows that simultaneity of muscle activity timing is well within the range of statistical certainty.

Feature	EMG	MKI
Detects both superficial and deep muscular activity	No	Yes
Operates without precise electrode placement	No	Yes
Eliminates electrodes & gel	No	Yes
Easily donnable by users	No	Yes
Useable in MRI	No	Yes
Useable raw signals	No	Yes

Future: By providing a non-invasive and readily usable means of detection of muscular volition, many diagnostic and rehabilitative procedures can be conducted more conveniently, more affordably, and requires less expertise to operate and interpret. We are developing the MKI for use in control of prosthetic devices, gait analysis and as biofeedback in stroke rehabilitation.